
PICM 20 DT electrical detection and stimulation



AURICULOTHERAPY

ACUPUNCTURE

REFLEXOLOGY

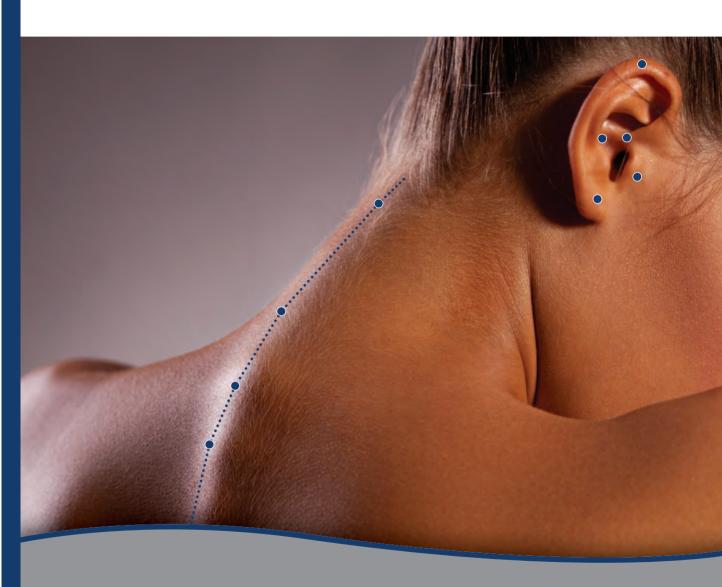



40 years of innovation and services dedicated to Auriculotherapy

Created by **Dr. Paul Nogier** in the 1950s, auriculotherapy has been recognised since the 1990s by the WHO. This technique is now practiced throughout the world.







The ASP® Original or Semi-Permanent Needle has been created and manufactured in France by Sedatelec in collaboration with Dr. Nogier.

From R&D, through design and development, to manufacture everything is "Made in France".

Sedatelec guarantees its products for 2 years and provides after-sales services from its premises in Lyon for up to 10 years after sales have been discontinued.

ISO 13485 CE0123



Premis 20 DT electrical detection and stimulation Grounding handle held by the patient Differential auriculotherapy electrode

Integrated command keyboard

Special acupuncture

ERT nozzle

Sedatelec was the original developer of the first auricular point detectors (Diascope®, Servoscope®, Agiscop®) and has concentrated all of its skills and expertise in the production of a new generation, with the **Premio 20**.

Revolutionary design

PRACTICAL: no cable or accessory part to install

ERGONOMIC: the first device with direct reading from the ear **ACCURATE:** 9 level differential detection with LED display

INNOVATIVE: frequency wobulation in stimulation mode between 1 and 100 Hz

SIMPLE: audible trigger threshold adjustment

COMFORTABLE: automatic adaptation of stimulation intensity




Detection

- Sufficiently low measurement current not to interfere with the point.
- Constant measurement electrode pressure on the epidermis.
- Highly accurate differential detection system (point and environment).
- Low (Gold) or high (Silver) impedance detection possible.
- Adjustable audible trigger threshold.
- Continuous measurement display on 9 levels.
- A grounding handle
 held by the patient which
 isolates the practitioner
 from the measurement
 circuit.

Differential detection

Measurement of the point environment



3 levels of led light indication



Automatic setting of the audible trigger threshold through measurement of the «O» point

D VERSION

DT VERSION

GT

GT



Stimulation

- Without taking your eyes off the point detected, simply pressing on the «D/T» button triggers stimulation by scanning the 7 Nogier* frequencies (1.14 Hz included).
- Automatic adaptation of stimulation intensity:
 no pain or burning sensation.
- Emission of a soft and fast «BLEEP» indicating to both patient and therapist that the stimulation is ongoing.
- Duration time set by a louder «BLEEP» every 30 seconds: average time required to incapacitate the point.
- Pressing again on «D/T» restarts detection without taking your eyes off the ear which is being investigated.





^{*}The Nogier frequencies are not recognised by Health Canada.



- Downward measurement of the impedance point.
- Special «Body» **ERT nozzle** with soft tip for perfect sliding.
- Progressive diode lighting proportional to the measurement.
- Direct instantaneous reading
 of the measurement on the stylet confirmed


by an «Audible BLEEP».

- Memorisation of the skin
 point detected with the lowest
 impedance.
- Reliability: grounding handle held by the patient isolates the practitioner from the measurement circuit.




Stimulation

- Without taking your eyes off the point detected, simply pressing on the «D/T» button triggers appropriate simulation for the patient's needs.
- INNOVATION: emission by frequency wobulation:
 - Alternate for harmonisation
 - Decreasing from 100 to 1 Hz in **dispersion**.
 - Rising between 1 and 100 Hz in tonification
- Option of working with Nogier* frequency scanning.
- Automatic adaptation of stimulation intensity: no pain or burning sensation.
- Emission of a regular «BLEEP» indicating to the patient and to the therapist that stimulation is ongoing.
- Duration time set by a louder «BLEEP» every 30 seconds.
- Pressing again on «D/T» restarts detection without taking your eyes off the ear which is being investigated.




HARMONISATION

This stimulation re-equilibrates the point and circulation in the meridian by alternating accelerations and decelerations of impulse frequency.



DISPERSION (100 to 1 Hz)

In a few seconds you will disperse the Qi and remove energy stasis. Dispersion is obtained by decreasing the impulse emission frequency.



TONIFICATION (1 to 100 Hz)

Rapid controlled stimulation of acupuncture points. Energising effect by accelerating impulse emission frequency.

«BLEEP» every 30 seconds

Effective, light and ergonomic

An ideal detector/stimulator for the consulting room and for portable use.



Distributor stamp

C € ₀₁₂₃ Manufactured in France



ELECTRO-THERAPEUTIC DEVICES INC.

70 Esna Park Drive, Unit 4, Markham, Ontario, Canada L3R 6E7 T:(905) 475-8344 F:(905) 475-5143

MORE THAN JUST ACUPUNCTURE